



100 Majestic Way, Bangor, PA 18013 / www.biospectra.us

TROMETHAMINE UNSPECIFIED DEGRADATION PRODUCTS VIA GC-FID

TABLE OF CONTENTS

1. PURPOSE:	3
2. SCOPE:	3
3. RESPONSIBILITIES:.....	3
4. REFERENCES:.....	3
5. MATERIALS AND EQUIPMENT:	3
6. METHOD PARAMETERS:.....	4
7. TESTING PROCEDURE:.....	5
8. CACULATIONS:	6
9. CHROMATOGRAMS:.....	6

The information contained herein is the confidential property of BioSpectra. The recipient is responsible for its safe-keeping and the prevention of unauthorized appropriation, use, disclosure and copying.

1. PURPOSE:

- 1.1. To provide Analysts with a procedure for determining Tromethamine unspecified degradation products determination by GC with FID determination.

2. SCOPE:

- 2.1. This analytical method applies to the Tromethamine unspecified degradation products determination via GC-FID.
- 2.2. This Tromethamine unspecified degradation products method was validated as a Category II quantitative analytical method.
- 2.3. The unspecified degradation product specification is not more than 0.03% each.
- 2.4. The method applies to the Tromethamine raw materials, in-process materials, stability materials and finished goods material analysis.

3. RESPONSIBILITIES:

- 3.1. The Director of Laboratory Systems is responsible for the control, training, implementation and maintenance of this procedure.
- 3.2. The analytical chemists or qualified designee is responsible for performing the testing in this procedure.
- 3.3. The analytical chemists performing this procedure with help from the Quality Control Manager if necessary, are responsible for documenting the results obtained from testing.
- 3.4. Safety: Standard laboratory safety regulations apply. Before working with any chemical and understand the Safety Data Sheet (SDS).

4. REFERENCES:

- 4.1. BSI-PRL-0688, Analytical Method Validation Protocol: Tromethamine Assay and degradation products determination via GC-FID
- 4.2. BSI-RPT-1373, Analytical Method Validation Report: Tromethamine Assay and degradation products determination via GC-FID
- 4.3. BSI-SOP-0098, Balance SOP
- 4.4. BSI-SOP-0126, Laboratory Notebooks
- 4.5. BSI-SOP-0134, Pipette SOP
- 4.6. BSI-SOP-0244, VWR Gravity Convection Operation and Calibration (Model Number 414005-106)
- 4.7. BSI-SOP-0436, Analytical Methods Validation Master Plan
- 4.8. Shimadzu QP2010S GC/MS SOP
- 4.9. USP NF <621>

5. MATERIALS AND EQUIPMENT:

5.1. Equipment:

- 5.1.1. Analytical Balance
- 5.1.2. Micropipettes
- 5.1.3. GC-MS
 - 5.1.3.1. Make: Shimadzu
 - 5.1.3.2. Model: GC-2010, equipped with FID detector.
- 5.1.4. GC Column: 30m RTX-5 Amino column 0.53mm ID 1.00 μ m film thickness
 - 5.1.4.1. Make: Restek
 - 5.1.4.2. Part Number: 12355
- 5.1.5. Laboratory Notebook

5.2. Reagents:

- 5.2.1. Purified Water/MilliQ Water
 - 5.2.1.1. Supplier: BioSpectra Inc.
 - 5.2.1.2. Meets or Exceeds USP Purified Water specification.
- 5.2.2. HPLC grade Methanol

5.3. Reference Standards:

- 5.3.1. Tromethamine Certified Reference Material (NIST)

5.4. Supplies:

- 5.4.1. Micropipette Tips
- 5.4.2. Class A volumetric flasks
- 5.4.3. Polypropylene transfer funnels or weighing boats

6. METHOD PARAMETERS:**6.1. GC-2010**

- 6.1.1. Column Oven Temperature: 150.0°C
- 6.1.2. Injection Mode: Split
- 6.1.3. Injector temperature 220.0°C
- 6.1.4. Detector temperature 275.0°C
- 6.1.5. Flow Control Mode: Linear Velocity
- 6.1.6. Pressure: 25.0 kPa
- 6.1.7. Total Flow: 23.3 mL/min (Impurity Level) and 236.8 mL/min (Assay Level)
- 6.1.8. Column Flow: 3.05 mL/min
- 6.1.9. Linear Velocity: 29.2 cm/sec
- 6.1.10. Purge Flow: 5.0 mL/min
- 6.1.11. Split Ratio: 5
- 6.1.12. High Pressure Injection: OFF
- 6.1.13. Carrier Gas Saver: OFF
- 6.1.14. Splitter Hold: OFF
- 6.1.15. Oven Temp Program:

Rate °C per Min	Temperature (°C)	Hold Time (min)
-	150.0	3.00
10.00	190.0	1.00
30.00	270.0	2.00
0.00	0.00	0.00

6.2. Ready Checks

- 6.2.1. Column Oven: YES
- 6.2.2. HS: NO
- 6.2.3. FID: YES
- 6.2.4. HS Carrier: NO
- 6.2.5. HS Purge: NO
- 6.2.6. APC1: YES
- 6.2.7. FID Makeup: YES
- 6.2.8. FID1 H2: YES
- 6.2.9. FID1 Air: YES
- 6.2.10. External Wait: NO
- 6.2.11. Auto Flame On: Yes
- 6.2.12. Auto flame Off: Yes
- 6.2.13. Reignite: Yes
- 6.2.14. Auto Zero After Ready: Yes

The information contained herein is the confidential property of BioSpectra. The recipient is responsible for its safe-keeping and the prevention of unauthorized appropriation, use, disclosure and copying.

6.2.15. Equilibrium Time: 0.0 min

7. TESTING PROCEDURE:

7.1. Solution Preparation

7.1.1. Note: Solutions may be scaled as needed

7.1.2. Diluent (6% Water in Methanol)

7.1.2.1. Pipette 3 mL of water into a 50 mL volumetric flask, dilute to volume with methanol and mix.

7.1.3. Sample Solutions

7.1.3.1. Accurately weigh 1.00 g of Tromethamine and transfer into a 50 mL volumetric flask, pipette in 3 mL of water, mix, dilute to volume with methanol and mix well. Sonicate if necessary to completely dissolve the Tromethamine.

7.1.4. Assay Standard Solution (20 mg/mL Tromethamine)

7.1.4.1. Accurately weigh 1.00 g of Tromethamine CRS and transfer into a 50 mL volumetric flask, pipette in 3 mL of water, mix, dilute to volume with methanol and mix well.

7.1.4.2. Sonicate if necessary to completely dissolve the Tromethamine.

7.1.5. Impurity-level Assay Standard Solution (0.2 mg/mL Tromethamine)

7.1.5.1. Pipette 5 mL of the Assay Standard solution into a 50 mL volumetric flask, add 3 mL of water, dilute to volume with methanol and mix well.

7.1.5.2. Pipette 5 mL of the solution prepared in Step 7.1.5.1. into a 50 mL volumetric flask, add 3 mL of water, dilute to volume with methanol, and mix well.

7.1.5.3. Label flask Impurity-level Assay Standard Solution

7.1.6. LOQ Solution (0.006 mg/mL Tromethamine)

7.1.6.1. Pipette 1.5 mL of the Impurity-level Assay Standard into a 50 mL volumetric flask, add 3 mL of water, dilute to volume with methanol and mix well.

7.1.6.2. Label flask: LOQ Solution

7.2. Injection Sequence

7.2.1. For Impurity Level Assay Standards samples and LOQ Solution inject with a split ratio of 5.

Sample ID	Number of Injections
System Suitability	
Diluent	≥1
LOQ	≥3
Impurity-level Assay Standard	5
Samples	
Samples	≤6 (1 injection each)
Diluent	1
Impurity-level Assay Standard (QC Check)	1
<ul style="list-style-type: none"> • Repeat the sample injection sequence if additional samples are to be analyzed • Samples may be substituted with diluent injections 	

7.3. System Suitability Criteria

System Suitability Parameter	Acceptance Criteria
The relative standard deviation of the Tromethamine peak from the first (5) injections of the Impurity-level Assay Standard solution.	NMT 20%
The average %Agreement between the first five (5) Impurity-level Assay Standard injections and each Impurity-level Assay Standard (QC check)	80% to 120%
Signal to noise ratio for the LOQ injection.	NLT 10:1


8. CALCULATIONS:

8.1. Unspecified Impurities


- 8.1.1. Report any peaks above the average peak area of the LOQ injections
- 8.1.2. Any peaks above the LOQ injections will result in the batch not meeting the specification limit of NMT 300 ppm.

9. CHROMATOGRAMS:

uV

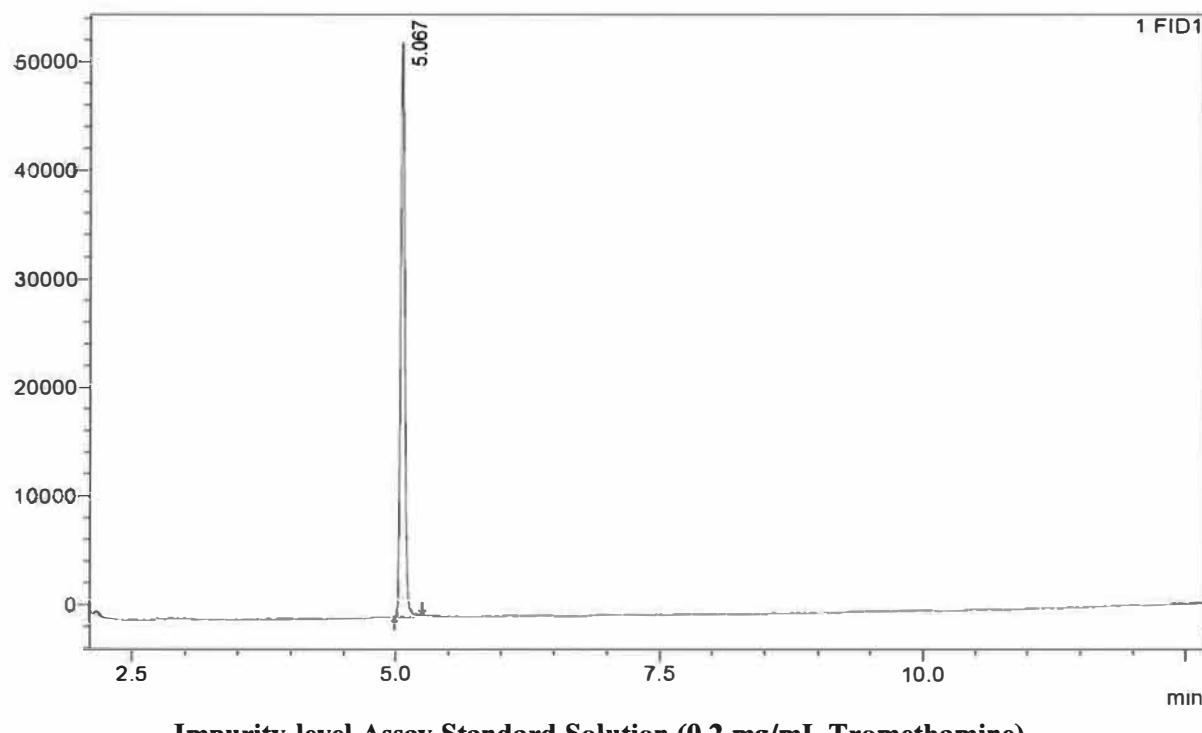


uV

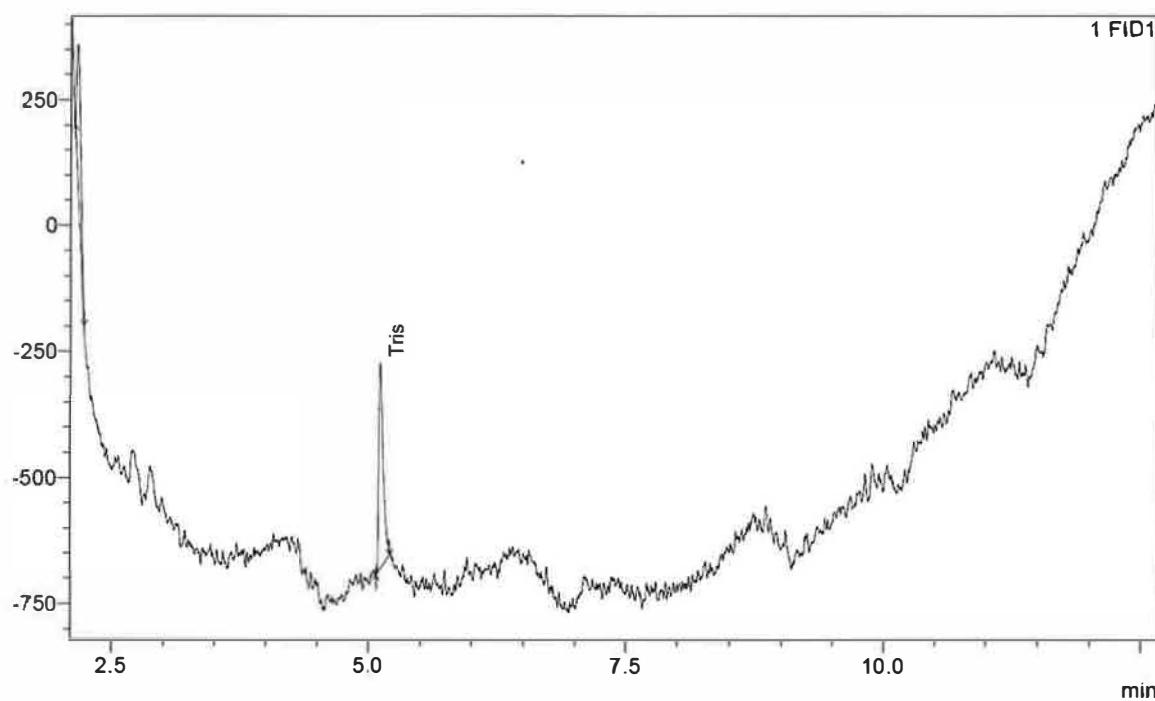

TRIS LOQ Solution (0.006 mg/mL Tromethamine)

uV

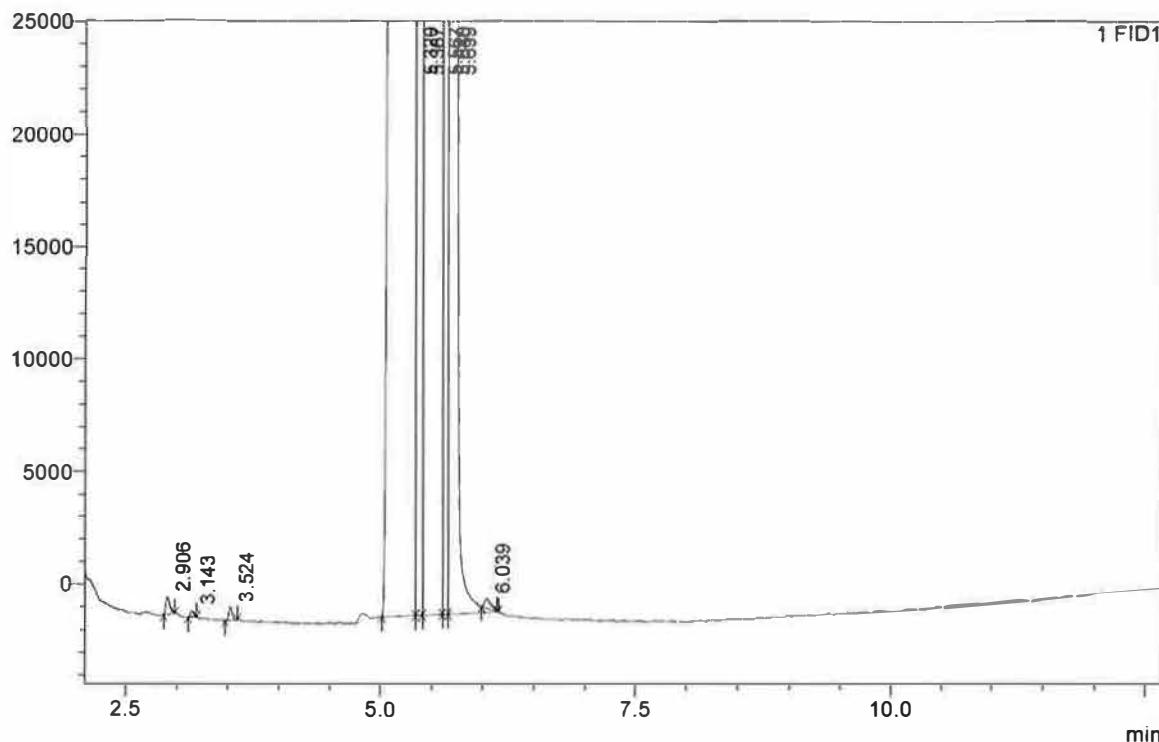

TRIS Sample Chromatogram

The information contained herein is the confidential property of BioSpectra. The recipient is responsible for its safe-keeping and the prevention of unauthorized appropriation, use, disclosure and copying.